



**EXECUTIVE SUMMARY**

DTE Energy’s Environmental Management and Resources (EMR) Field Services Group performed a Response Correlation Audit (RCA) on the Particulate Matter Continuous Emissions Monitoring System (PM CEMS). The RCA was performed on the EUBOILER#3 exhaust stack located at the River Rouge Power Plant, in River Rouge, Michigan. Testing is required by 40 CFR Part 63 Subpart UUUUU and Michigan Department of Environment, Great Lakes, and Energy (EGLE) Renewable Operating Permit No. MI-ROP-B2810-2012b. Testing was conducted between June 6-11, 2019 in accordance with Procedure 2 of 40 CFR Part 60, Appendix F.

Criteria for acceptable RCA results is located in Procedure 2 Sec 10.4(5)(i-ii) and is summarized below.

	PM CEMS (mg/acm)	RM PM (mg/acm)	PM CEMS (correlation)	Correlation (-25% Emission Limit)	Correlation (+25% Emission Limit)
Run 1	0.3	3.48	4.4	-0.31	9.19
Run 2	0.1	0.99	4.4	-0.37	9.13
Run 3	0.1	0.67	4.4	-0.37	9.13
Run 4	0.1	1.62	4.4	-0.37	9.13
Run 5	0.0	0.76	4.3	-0.40	9.10
Run 6	31.7	12.0	13.7	8.92	18.42
Run 7	36.3	12.2	15.0	10.27	19.77
Run 8	31.2	14.9	13.5	8.77	18.27
Run 9	30.8	11.8	13.4	8.65	18.15
Run 10	35.7	13.5	14.8	10.09	19.59
Run 11	80.5	25.2	28.0	23.26	32.76
Run 12 <sup>1</sup>	87.6	23.5	30.1	25.35	34.85
Run 13 <sup>1</sup>	86.9	23.8	29.9	25.15	34.65
Run 14 <sup>1</sup>	85.9	21.5	29.6	24.85	34.35
Run 15	77.9	21.2	27.2	22.50	32.00
<b>PM CEMS &lt; Greatest PM CEMS Response on correlation regression line</b>				<b>≤98.5 mg/acm</b>	<b>Pass</b>
<b>9 of 12 PM CEMS and RM w/in 25% of numerical emission limit on correlation regression line</b>					<b>Pass</b>

<sup>(1)</sup> Three runs were discarded due to poor correlation



## **1.0 INTRODUCTION**

DTE Energy's Environmental Management and Resources (EMR) Field Services Group performed a Response Correlation Audit (RCA) on the Particulate Matter Continuous Emissions Monitoring System (PM CEMS). The RCA was performed on the EUBOILER#3 exhaust stack located at the River Rouge Power Plant, in River Rouge, Michigan. The testing is required by 40 CFR Part 63 Subpart UUUUU and Michigan Department of Environment, Great Lakes, and Energy (EGLE) Renewable Operating Permit No. MI-ROP-B2810-2012b. Testing was conducted between June 6-11, 2019 in accordance with Procedure 2 of 40 CFR Part 60, Appendix F.

Criterion for acceptable RCA results are located in Part 60, Appendix F Procedure 2 Sec 10.4(6)(i-ii).

The fieldwork was performed in accordance with EPA Reference Methods and EMR's Intent to Test.<sup>1,2</sup> The following EMR Field Services personnel participated in the testing program: Mr. Jason Logan, Environmental Specialist, Mr. Mark Westerberg, Senior Environmental Specialist, Mr. Frank Kurta, Environmental Technician, and Mr. Kenneth St. Amant, Senior Environmental Technician. Mr. Logan was the project leader. Coordination with the facility was performed by Ms. Tanecia Wilson, Associate Engineer.

## **2.0 SOURCE DESCRIPTION**

The River Rouge Power Plant (RRPP), located at 1 Belanger Park Dr. River Rouge, Michigan, employs the use of one coal-fired boiler. EUBOILER#3 is a Foster-Wheeler Boiler, nominally rated at 278 GMW. Particulate emissions from EUBOILER#3 are controlled via a Wheelabrator-Fry electrostatic precipitator (ESP). The air pollution control equipment has a designed collection efficiency of 99.9%.

The boiler is equipped with a Dry Sorbent Injection (DSI) and Activated Carbon Injection (ACI) air quality control system. The DSI system is used to control acid gases from the unit. Trona is received at the plant where inline mills further refine the Trona. The ACI system is used to control Mercury emissions.

The coal blend for EUBOILER#3 was 100% low-sulfur western (LSW). Testing was performed on EUBOILER#3 while operating at normal load conditions, per Subpart

---

<sup>1</sup> EGLE, Test Plan, Submitted October 26, 2018. (Attached-Appendix A)

<sup>2</sup> EGLE, Approval Letter, Received January 11, 2019. (Attached-Appendix A)



River Rouge Power Plant utilizes Sick AG Maihak SP100 dust measuring systems. The analyzers utilize a measuring technique based off scattered light principal. The SP100 model is specific for low to medium dust collections. The following unit was audited:

Unit	Analyzer	Manufacturer/Model	Analyzer Range	Serial Number
EUBOILER#3	PM	Sick/ Maihak SP100	200 mg/acm	15318415

### 3.0 SAMPLING AND ANALYTICAL PROCEDURES

DTE Energy obtained emissions measurements in accordance with procedures specified in the USEPA *Standards of Performance for New Stationary Sources*. The sampling and analytical methods used in the testing program are indicated in the table below

Sampling Method	Parameter	Analysis
USEPA Methods 1-2	Exhaust Gas Flow Rates	Field data analysis and reduction
USEPA Method 3A	O <sub>2</sub> & CO <sub>2</sub>	Instrumental Analyzer Method
USEPA Method 4	Moisture Content	Field data analysis and reduction
USEPA Method 5 – MATS Modified	Particulate Matter (Non-Sulfuric Acid)	Gravimetric Analysis

### 3.1 **STACK GAS VELOCITY AND FLOWRATES (USEPA Methods 1-2)**

#### 3.1.1 **Sampling Method**

Stack gas velocity traverses were conducted in accordance with the procedures outlined in USEPA Method 1, “Sample and Velocity Traverses for Stationary Sources,” and Method 2, “Determination of Stack Gas Velocity and Volumetric Flowrate.” Four (4) sampling ports were utilized on each unit’s exhaust stack, sampling at six (6) points per port for a total of twenty-four (24) points. Velocity traverses were conducted simultaneously with the particulate sampling. See Figure 1 for a diagram of the traverse/sampling points used.

# DTE

Cyclonic flow checks were performed on each stack during the initial flow monitor certification RATAs. Testing at the sampling location demonstrated that no cyclonic flow was present at either location. No changes to the stacks have occurred since the cyclonic flow checks were performed. Additionally, verifications of null angle at  $0^\circ$  were observed while performing static pressure checks.

### **3.1.2 Method 2 Sampling Equipment**

The EPA Method 2 sampling equipment consisted of a 0-10" incline manometer, S-type Pitot tube ( $C_p = 0.84$ ) and a Type-K calibrated thermocouple.

## **3.2 OXYGEN & CARBON DIOXIDE (USEPA Method 3A)**

### **3.2.1 Sampling Method**

Oxygen ( $O_2$ ) and carbon dioxide ( $CO_2$ ) emissions were evaluated using USEPA Method 3A, "Gas Analysis for Carbon Dioxide, Oxygen, Excess Air, and Dry Molecular Weight (Instrumental Analyzer Method)". The analyzers utilize paramagnetic sensors.

### **3.2.2 $O_2/CO_2$ Sampling Train**

The EPA Method 3A sampling system (Figure 2) consisted of the following:

- (1) PTFE sampling line (collecting gas sample from the dry gas meter exhaust)
- (2) 10 liter Tedlar bag
- (3) Servomex 1400  $O_2/CO_2$  gas analyzer
- (4) Appropriate USEPA Protocol 1 calibration gases

### **3.2.3 Sampling Train Calibration**

The  $O_2$  and  $CO_2$  analyzers were calibrated per procedures outlined in USEPA Methods 3A. Zero, span, and mid-range calibration gases were introduced directly into the analyzer to verify the instruments linearity, prior to sampling, and again at the completion of each test run.

## **3.3 MOISTURE DETERMINATION (USEPA Method 4)**

### **3.3.1 Sampling Method**

Determination of the moisture content of the exhaust gas was performed using USEPA Method 4, "Determination of Moisture Content in Stack Gases". The moisture was collected in glass impingers as a component of the Method 5

(Modified) sampling train, and the percentage of water was then derived from calculations outlined in USEPA Method 4.

### 3.4 PARTICULATE MATTER (USEPA Method 5 – MATS Modified)

#### 3.4.1 *Filterable Particulate Sampling Method*

USEPA Method 5 – MATS Modified, “Determination of Particulate Emissions from Stationary Sources” was used to measure the filterable (front-half) particulate emissions (see Figure 3 for a schematic of the sampling train). Fifteen (15), 60-minute test runs were conducted.

The Method 5 – MATS Modified modular isokinetic stack sampling system consisted of the following:

- (1) PTFE coated stainless-steel button-hook nozzle
- (2) Heated glass-lined probe
- (3) Heated 3” glass filter holder with a quartz filter  
(Maintained at a temperature of  $320 \pm 25$  °F)
- (4) Set of impingers for the collection of condensate for moisture determination
- (5) Length of sample line
- (6) Environmental Supply® control case equipped with a pump, dry gas meter, and calibrated orifice.

The quartz filters used in the sampling were initially baked for 3 hours at 320 °F, desiccated for 24 hours and weighed to a constant weight as described in Method 5 - MATS Modified to obtain the initial tare weight.

After completion of the final leak test for each test run, the filter was recovered, and the probe, nozzle and the front half of the filter holder assembly were brushed and rinsed with acetone. The acetone rinses were collected in a pre-cleaned sample container. The container was labeled with the test number, test location, test date, and the level of liquid marked on the outside of the container. Immediately after recovery, the sample containers were placed in a cooler for storage.

At the laboratory, the acetone rinses were transferred to clean pre-weighed beakers, and evaporated to dryness at ambient temperature and pressure. The beakers and filters were desiccated for 24 hours and weighed to a constant weight (within 0.5

# DTE

mg). The data sheets containing the initial and final weights on the filters and beakers can be found in Appendix C.

Collected field blanks consisted of a blank filter and acetone solution blank. The acetone blank was collected from the rinse bottle used in sample recovery. The blank filter and acetone were collected and analyzed following the same procedures used to recover and analyze the field samples. Field data sheets for the Method 5 - MATS Modified sampling can be found in Appendix B.

### **3.4.2 Quality Control and Assurance**

All sampling and analytical equipment was calibrated per the guidelines referenced in EPA Method 5 – MATS Modified. All calibration data for Methods 1-5 is in Appendix D.

### **3.4.3 Data Reduction**

The filterable PM emissions data collected during the testing were calculated and reported as mg/acm.

## **4.0 OPERATING PARAMETERS**

The test program included the collection of PM CEMs emission data and Load during each PM emissions test. Data collected during the testing is presented in Appendix E.

## **5.0 DISCUSSION OF RESULTS**

Table 1 presents the Reference Method particulate emission testing results (RM PM), raw particulate matter continuous emissions monitoring system (PM CEMS) results, unit load, and PM range designation for each test. It also identifies which test runs were excluded. Results from twelve of the fifteen total test runs were imprinted on the curve developed from the original PS-11 testing. Particulate emissions are presented in milligram per actual cubic meter (mg/acm).

In order to pass an RCA, All of the following criteria must be met: Procedure 2 10.4(5)(i-ii).

- i) For 12 data points, minimum, the PM CEMS Correlation value can be no greater than the greatest PM CEMS Correlation value used to develop your correlation curve.
- ii) At least 75% of a minimum number of 12 sets of PM CEMS and Reference Method measurements must fall within the same specified area on a graph of

# DTE

the correlation regression line. The specified area on the graph of the correlation regression line is defined by two lines parallel to the correlation regression line, offset at a distance of  $\pm 25\%$  of the numerical emission limit value from the correlation regression line.


The EUBOILER#3 RCA testing met all criteria.


Table 2 presents a graph which includes the RCA test points overlaying the curve from the PS-11 testing.



6.0 CERTIFICATION STATEMENT

"I certify that I believe the information provided in this document is true, accurate, and complete. Results of testing are based on the good faith application of sound professional judgment, using techniques, factors, or standards approved by the Local, State, or Federal Governing body, or generally accepted in the trade."

  
\_\_\_\_\_  
Jason Logan, QSTI

This report prepared by:   
\_\_\_\_\_  
Mr. Jason Logan, QSTI  
Environmental Specialist, Field Services Group  
Environmental Management and Resources  
DTE

This report reviewed by: \_\_\_\_\_  
Mr. Thomas Durham  
Manager, Field Services Group  
Environmental Management and Resources  
DTE



**DTE**

**RESULTS TABLES**



**TABLE NO. 1**  
**RCA TEST RESULTS**  
**PARTICULATE MATTER CONTINUOUS EMISSIONS MONITORING SYSTEM**  
**River Rouge Power Plant - EUBOILER#3 Stack**  
**June 6-11, 2019**

Test ID	Date (2019)	Test Time DAHS (24 hour)	Unit Load (GMW)	PM CEMS (mg/acm) <sup>1</sup>	PM RM (mg/acm) <sup>1</sup>	PM Load Range
PM-1	6-Jun	7:44-8:52	215	0.3	3.48	Low
PM-2	6-Jun	9:17-10:23	216	0.1	0.99	Low
PM-3	6-Jun	10:39-11:46	216	0.1	0.67	Low
PM-4	6-Jun	12:02-13:08	166	0.1	1.62	Low
PM-5	6-Jun	13:24-14:36	154	0.0	0.76	Low
PM-6	7-Jun	10:58-12:06	214	31.7	12.0	Mid
PM-7	7-Jun	12:21-13:26	214	36.3	12.2	Mid
PM-8	10-Jun	8:23-9:30	151	31.2	14.9	Mid
PM-9	10-Jun	9:48-10:53	151	30.8	11.8	Mid
PM-10	10-Jun	11:07-12:12	151	35.7	13.5	Mid
PM-11	11-Jun	8:00-9:04	182	80.5	25.2	High
PM-12	11-Jun	9:18-10:25	182	87.6	23.5	High
PM-13	11-Jun	10:37-11:41	182	86.9	23.8	High
PM-14	11-Jun	11:58-13:03	182	85.9	21.5	High
PM-15	11-Jun	13:15-14:19	182	77.9	21.2	High

<sup>1</sup>milligrams per actual cubic meter (@ 160°C)


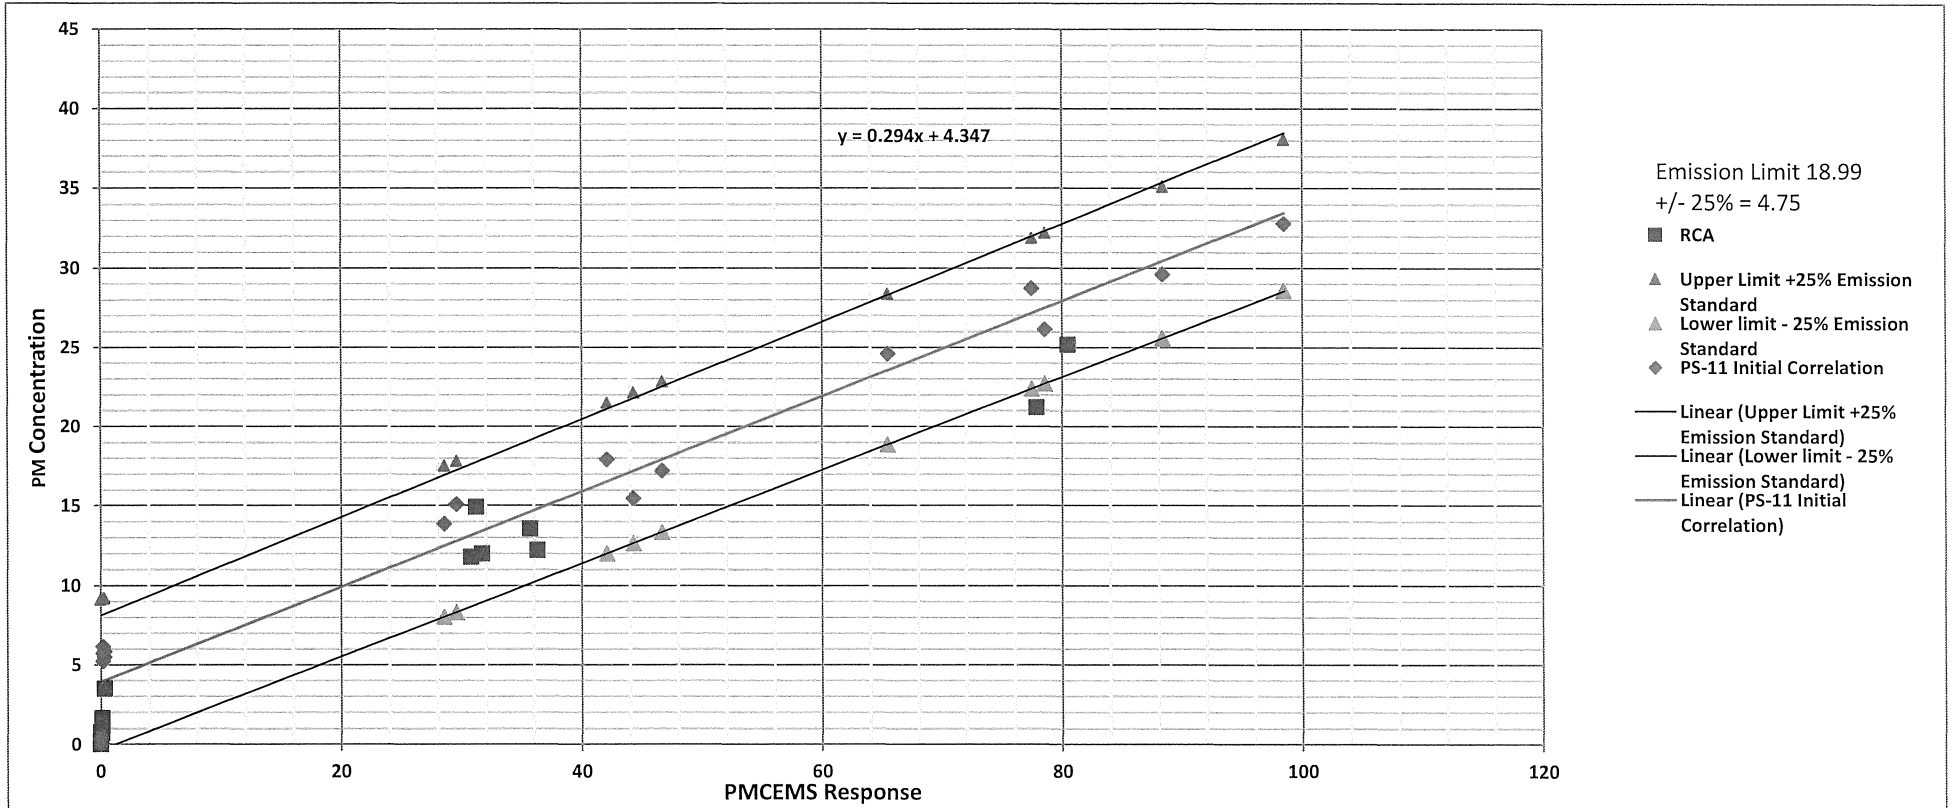
 = Data Not Included in the RCA correlation graph


TABLE No. 2  
 River Rouge Power Plant  
 UNIT 3  
 PM CEMS RCA  
 SUMMARY GRAPH  
 June 6-11, 2019



**DTE**

**FIGURES**


Figure 1 - Sampling Location  
River Rouge Power Plant - EUBOILER#3

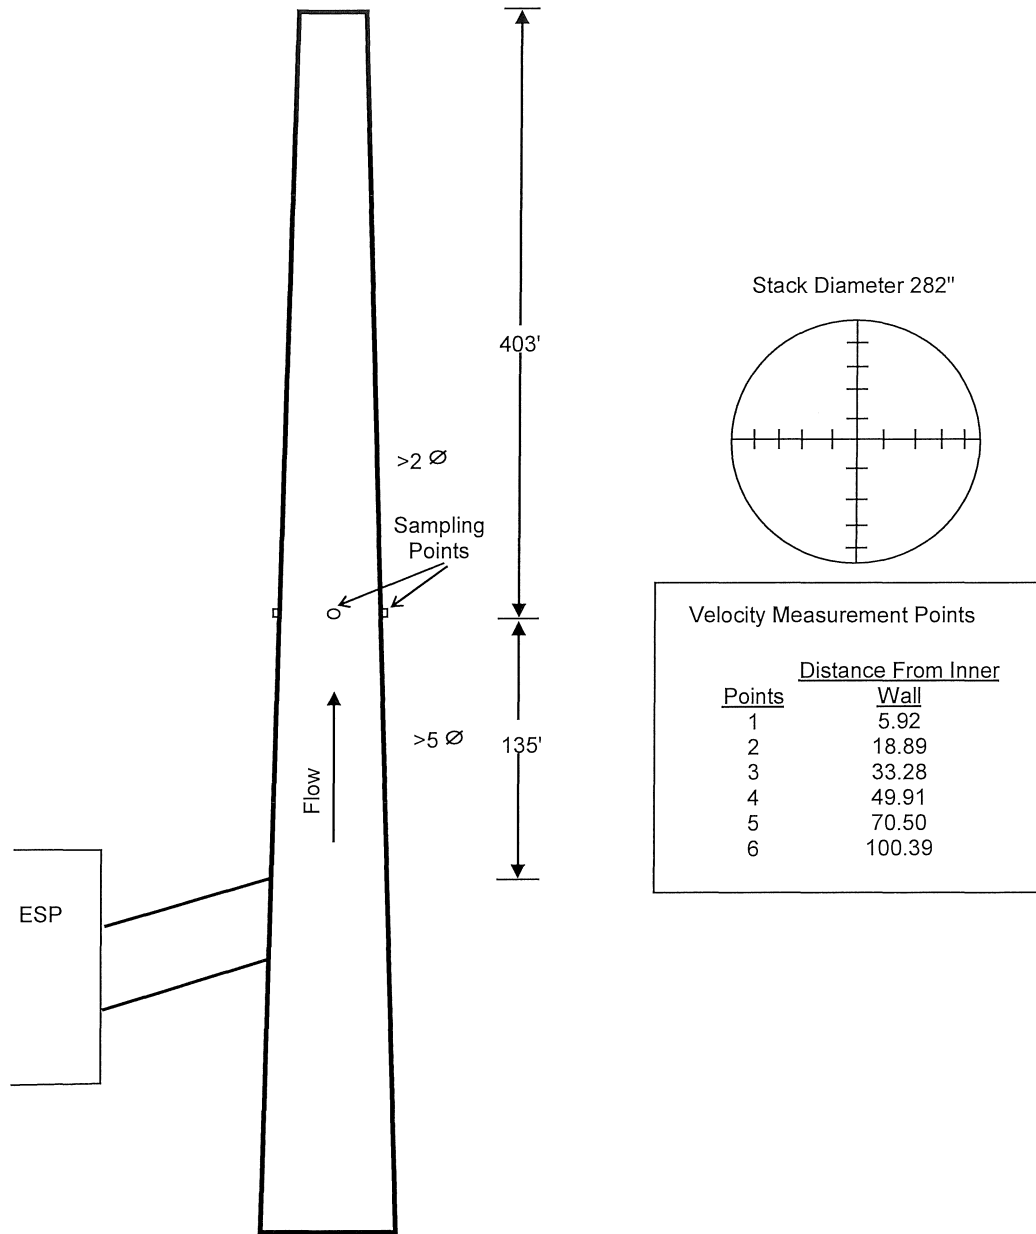

Velocity Measurement Points

<u>Points</u>	<u>Distance From Inner Wall</u>
1	5.92
2	18.89
3	33.28
4	49.91
5	70.50
6	100.39

Figure 2 - EPA Method 3A  
River Rouge Power Plant - EUBOILER#3

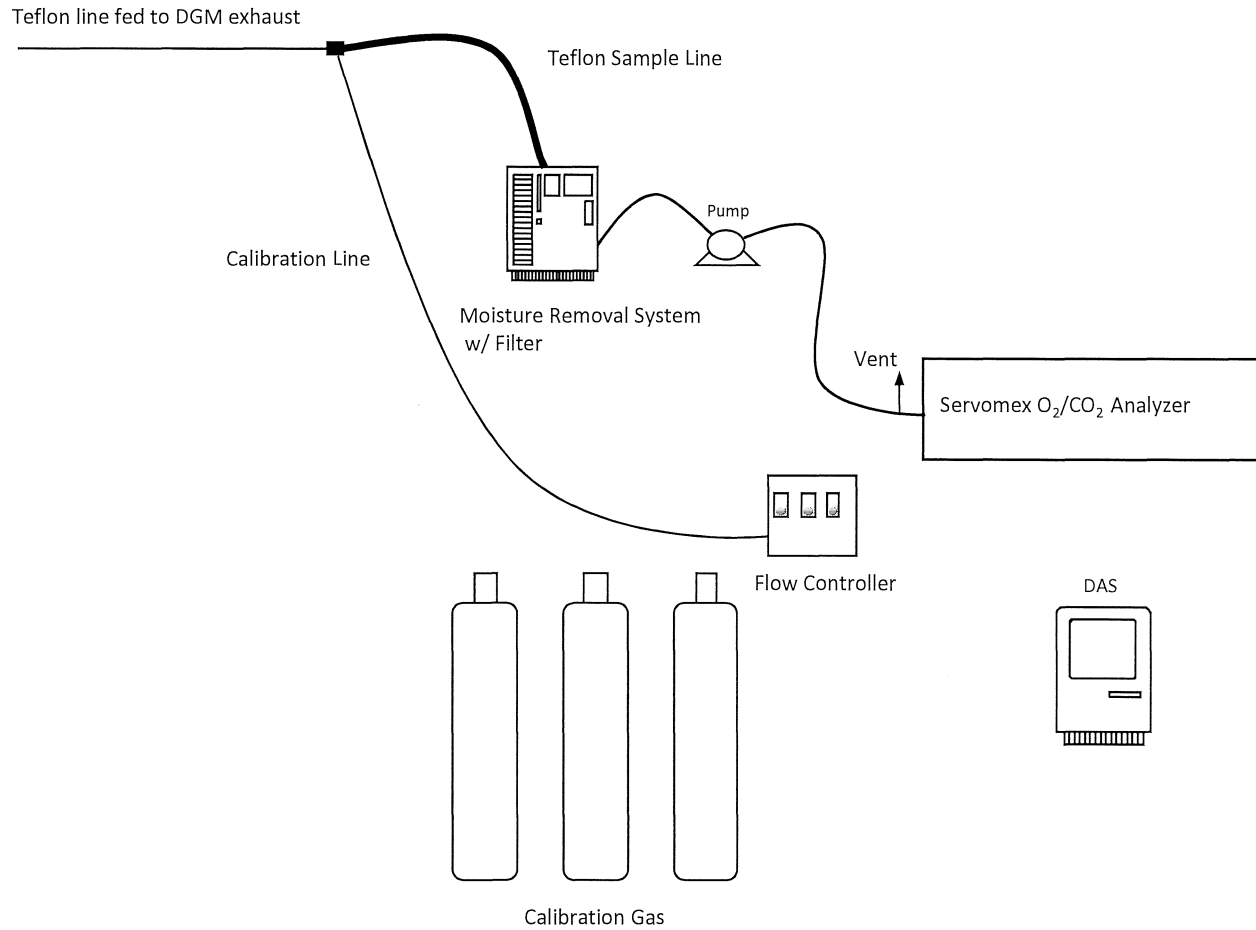

# DTE

Figure 3 - EPA Method 5 MATS Modified  
River Rouge Power Plant - EUBOILER#3

